
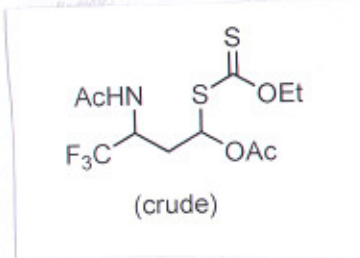


HL 50-861-V1-V1  
LAU-LA-198-05 1H

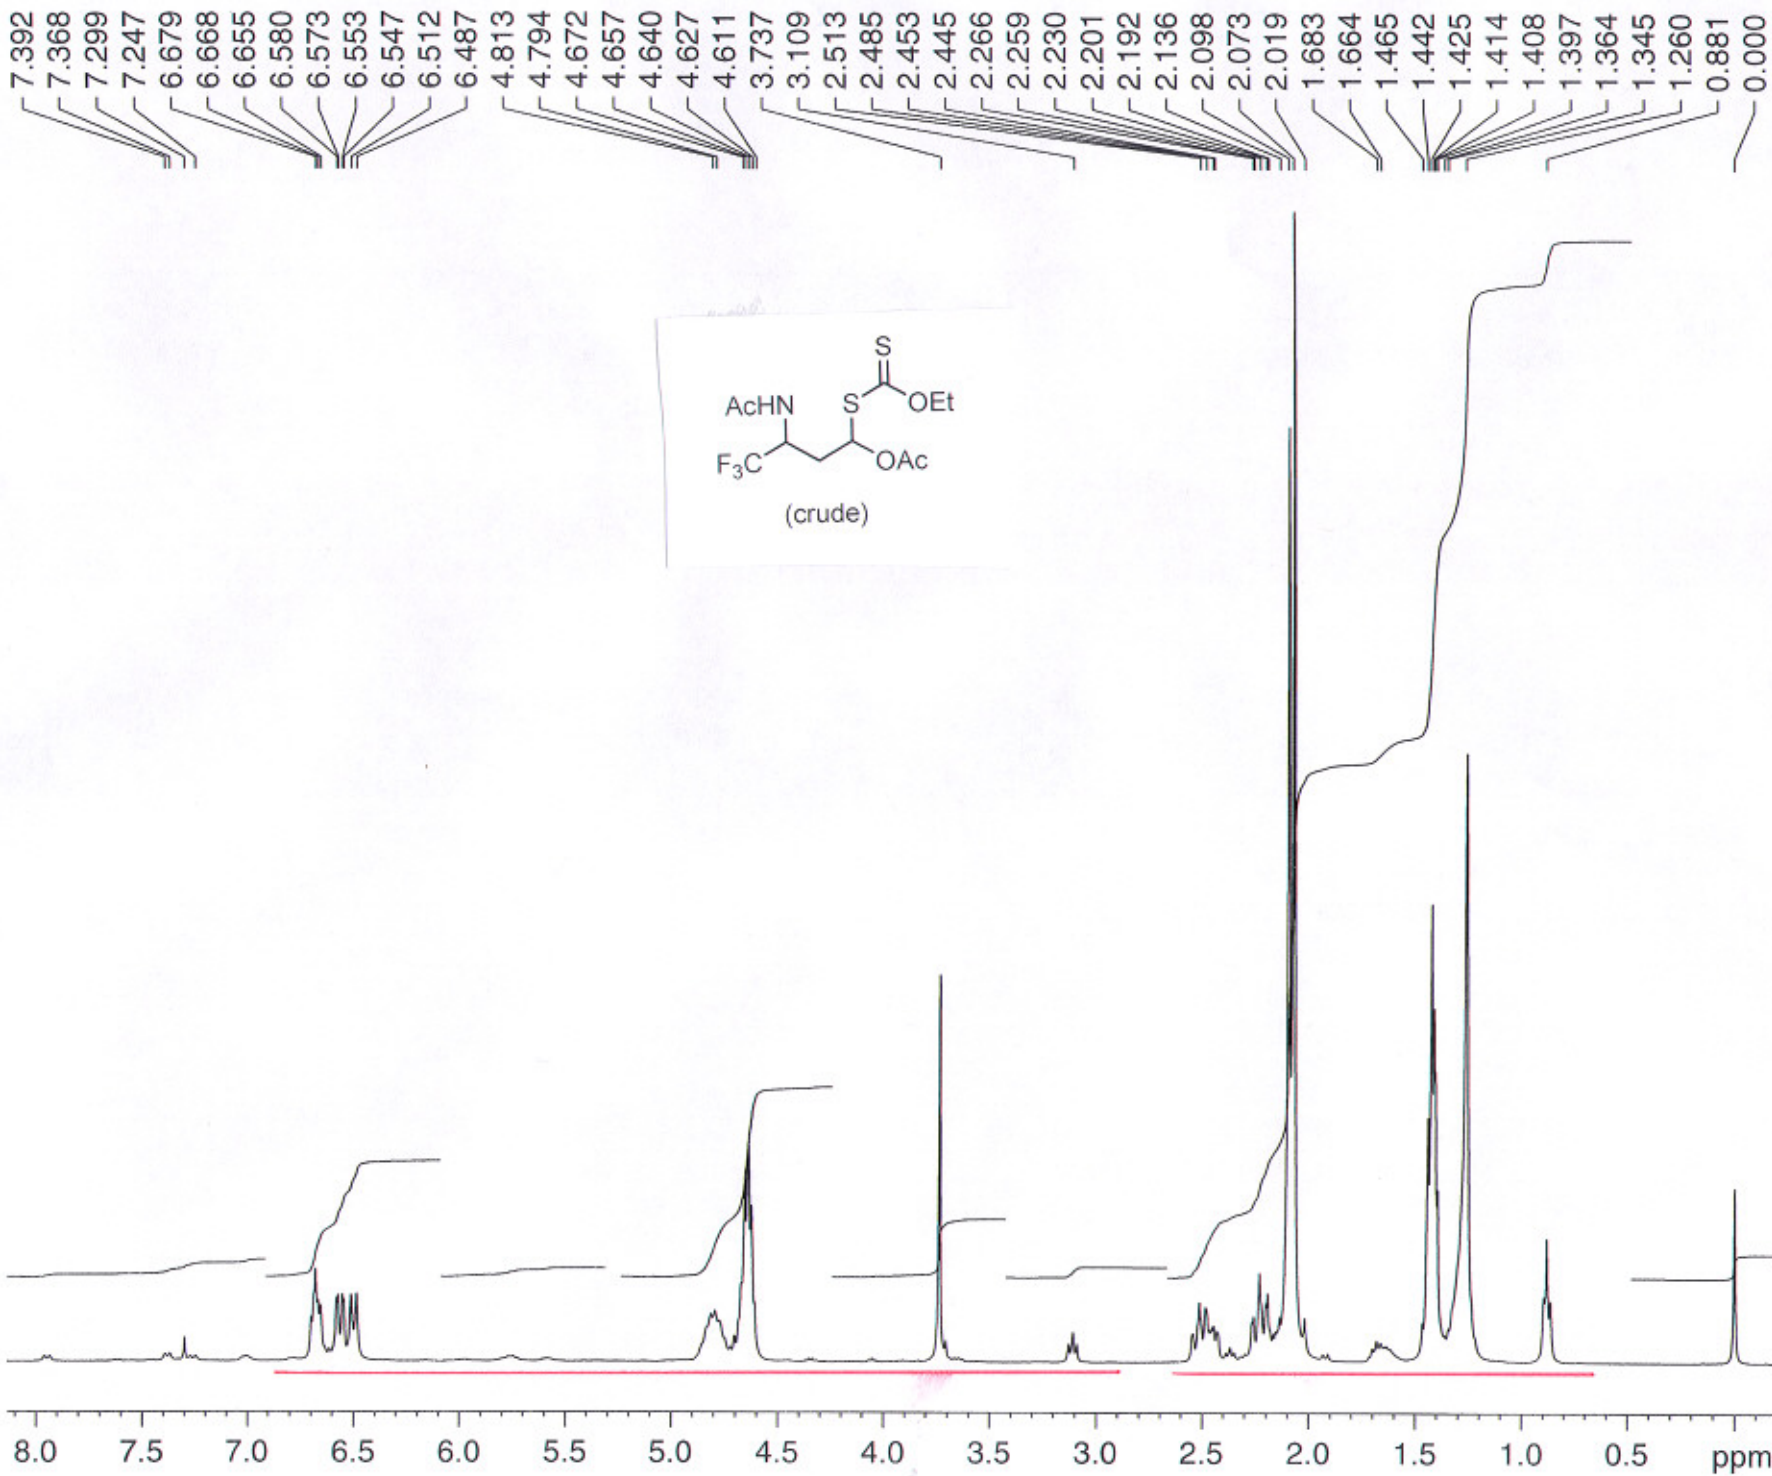

Current Data Parameters  
NAME mz08007  
EXPNO 10  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20060308  
Time 10.20  
INSTRUM av400  
PROBHD 5 mm BBO BB-1H  
PULPROG zg30  
TD 65536  
SOLVENT CDCl3  
NS 32  
DS 8  
SWH 8278.146 Hz  
FIDRES 0.126314 Hz  
AQ 3.9584243 sec  
RG 25.4  
DW 60.400 usec  
DE 6.50 usec  
TE 303.0 K  
D1 0.00300000 sec

===== CHANNEL f1 =====  
NUC1 1H  
P1 9.25 usec  
PL1 0.00 dB  
SFO1 400.1324710 MHz

F2 - Processing parameters  
SI 32768  
SF 400.1299943 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 2.00