



OS
C13CPD CDC13 {Z:\data} ueda 30

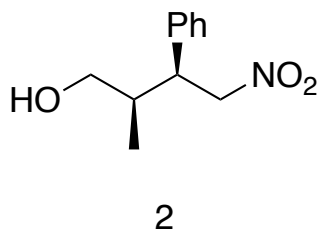

— 137.7271
128.6790
128.3456
127.5864
78.7723
77.2354
77.0239
76.8122
— 65.6770
— 46.2414
— 38.3737
— 14.0960
— 0.0057

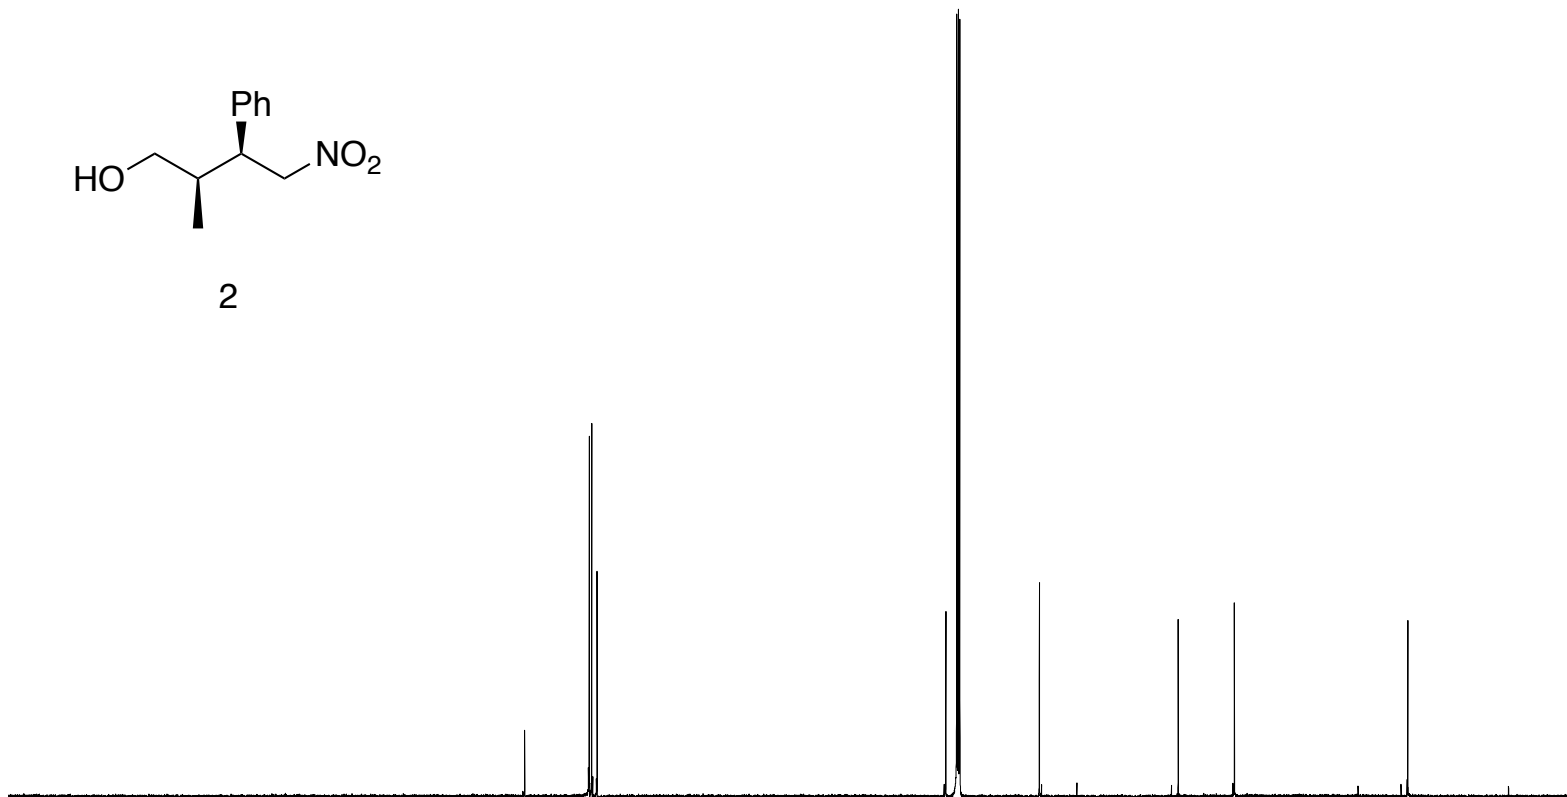

Current Data Parameters
NAME OS
EXPNO 41
PROCNO 1

F2 - Acquisition Parameters
Date_ 20170705
Time_ 11.28
INSTRUM spect
PROBHD 5 mm CPPBBO BB
PULPROG zgpg30
TD 65536
SOLVENT CDC13
NS 256
DS 4
SWH 36057.691 Hz
FIDRES 0.550197 Hz
AQ 0.9087659 sec
RG 175.56
DW 13.867 use
DE 18.00 use
TE 300.0 K
D1 2.00000000 sec
D11 0.03000000 sec
TD0 1

==== CHANNEL f1 =====
SFO1 150.9178981 MHz
NUC1 13C
P1 10.00 use
PLW1 70.00000000 W

==== CHANNEL f2 =====
SFO2 600.1324005 MHz
NUC2 1H
CPDPRG[2] waltz16
PCPD2 70.00 use
PLW2 14.00000000 W
PLW12 0.64286000 W
PLW13 0.32335001 W

F2 - Processing parameters
SI 32768
SF 150.9028095 MHz
WDW EM
SSB 0
LB 1.00 Hz
GB 0
PC 1.40

200 190 180 170 160 150 140 130 120 110 100 90 80 70 60 50 40 30 20 10 0 ppm