


7.742  
 7.728  
 7.451  
 7.435  
 7.423  
 7.411  
 7.397  
 7.382  
 7.259

2.380  
 2.261

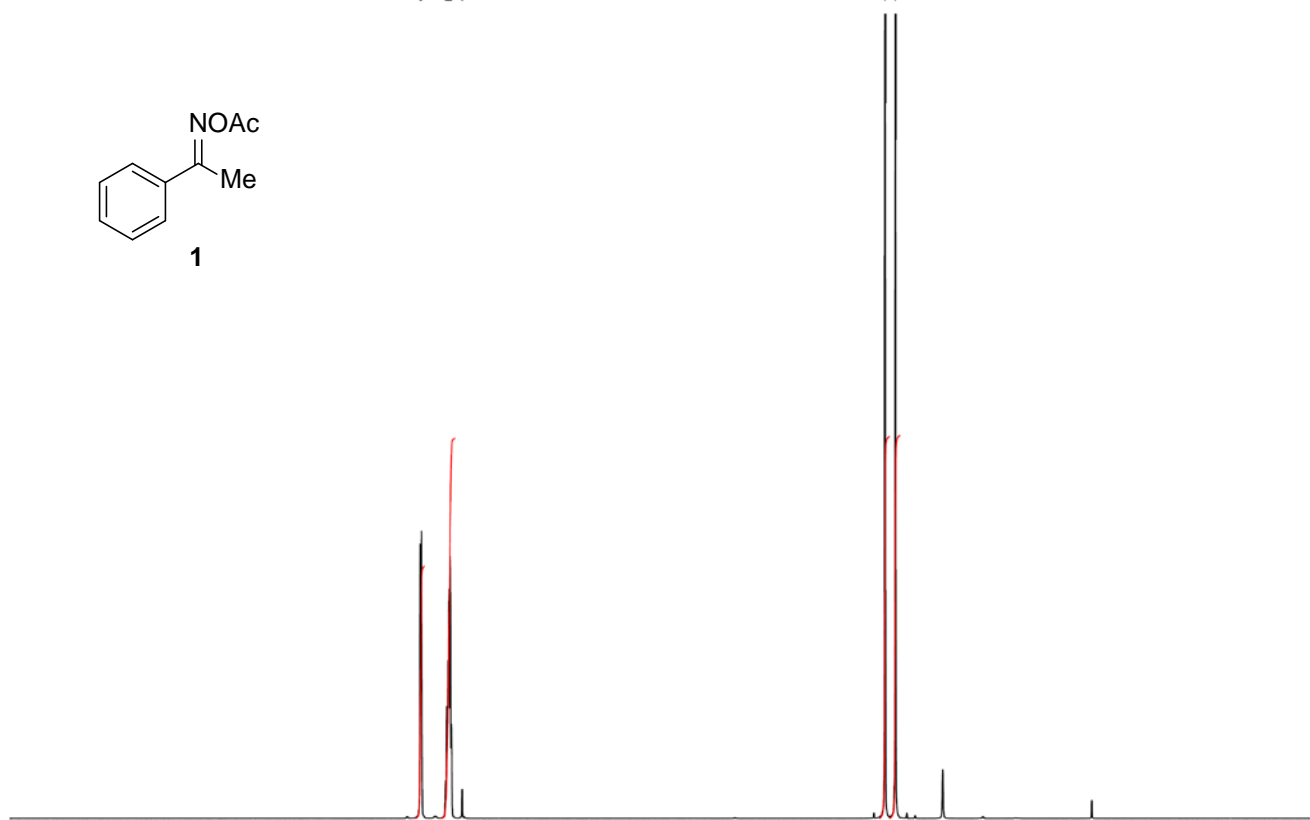

12 11 10 9 8 7 6 5 4 3 2 1 0 -1 ppm

1.98  
2.99

3.00  
3.01



Current Data Parameters  
 NAME srl-00209-1  
 EXPNO 1  
 PROCNO 1

F2 - Acquisition Parameters  
 Date 20170922  
 Time 17.48  
 INSTRUM spect  
 PROBHD 5 mm PABBO BB-  
 PULPROG zg10  
 TD 32768  
 SOLVENT CDCl3  
 NS 16  
 DS 0  
 SWH 7500.000 Hz  
 FIDRES 0.228882 Hz  
 AQ 2.1845334 sec  
 RG 144  
 DW 66.667 usec  
 DE 6.50 usec  
 TE 299.0 K  
 D1 1.00000000 sec  
 TD0 1

===== CHANNEL f1 =====  
 SF01 500.1325007 MHz  
 NUC1 1H  
 P1 11.75 usec  
 PLW1 18.39999962 W

F2 - Processing parameters  
 SI 16384  
 SF 500.1300116 MHz  
 WDW EM  
 SSB 0  
 LB 0.30 Hz  
 GB 0  
 PC 1.00

