
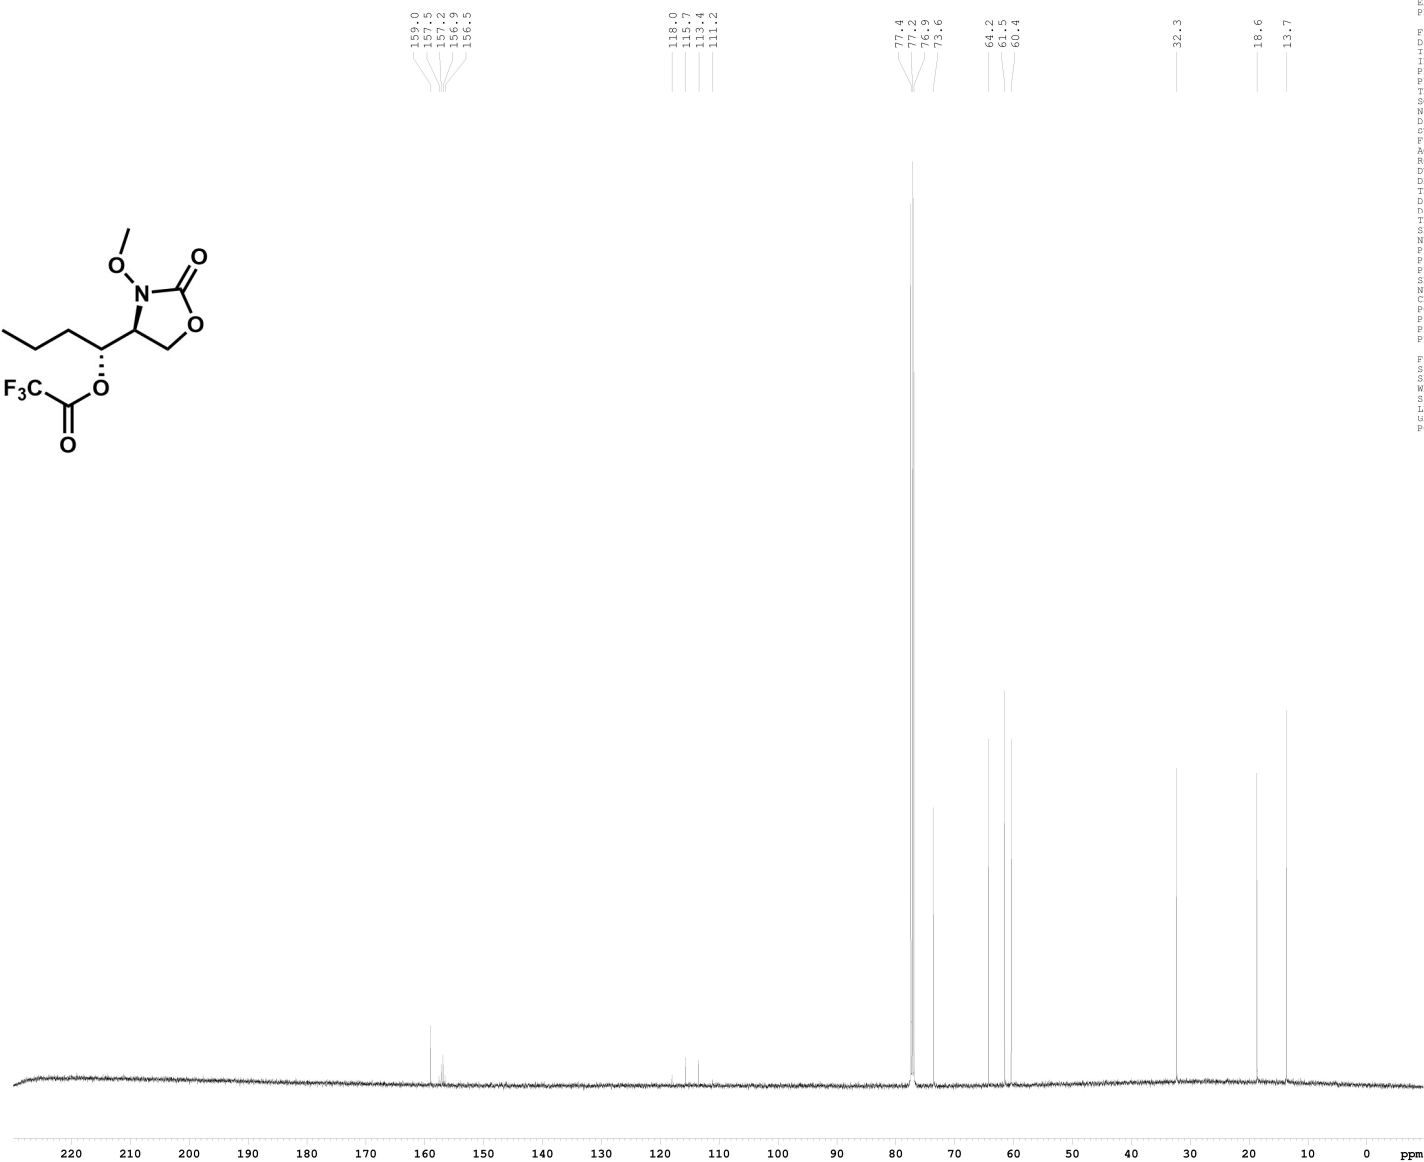




Current Data Parameters
 NAME 7E-3-604-pr
 EXPNO 2
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20250611
 Time 21:37 h
 INSTRUM AvanceNeo 500
 PROBHD Z168790_0022 (CP1.1 TCI 5h
 PULPROG zgpg30
 TD 65060
 SOLVENT CDCl3
 NS 1024
 DS 4
 SWH 30120.482 Hz
 FIDRES 0.923529 Hz
 AQ 1.0799960 sec
 RG 101
 DW 16.600 usec
 DE 18.00 usec
 TE 298.0 K
 D1 0.25000000 sec
 D11 0.03000000 sec
 TD0 1
 SFO1 125.7716219 MHz
 NUC1 13C
 P0 3.54 usec
 P1 10.62 usec
 PLW1 96.95098877 W
 SFO2 500.1320005 MHz
 NUC2 1H
 CFPD2 waltz165
 PLW2 9.26000023 W
 PLW12 0.09329600 W
 PLW13 0.04685200 W

F2 - Processing parameters
 S1 32768
 SF 125.7577719 MHz
 MDW EM
 SSB 0
 LB 1.00 Hz
 GB 0
 PC 1.40